
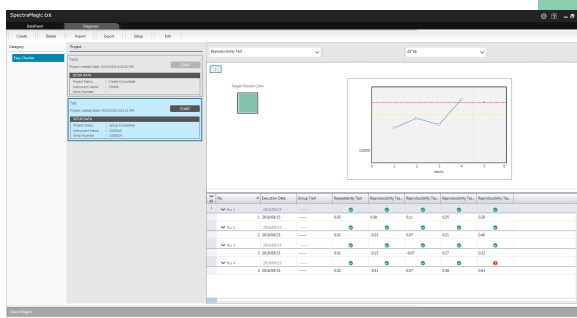
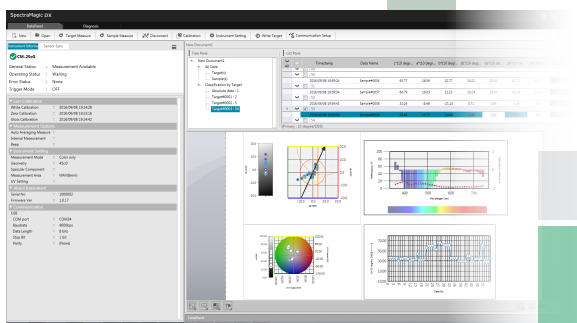


New QC software with a new Instrument Diagnosis function !

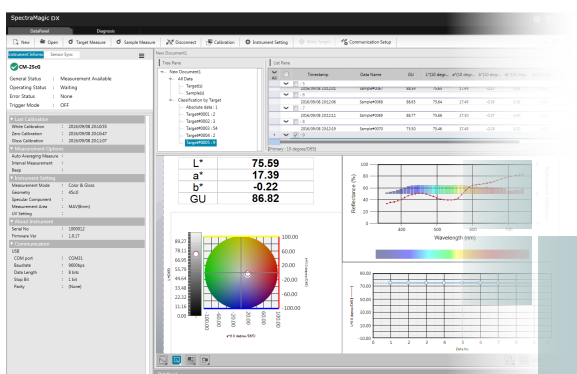

Compatible instruments :

Spectrophotometer CM-25cG
 Spectrophotometer CM-M6
 Spectrophotometer CM-2500c

Instrument Diagnosis function :

(Spectrophotometer CM-25cG, CM-M6)

A new function to help ensure continued high instrument performance such as repeatability, reproducibility, or lamp output by measuring your color tiles etc.

Minimum Computing Requirements	
OS	Windows® 7 Pro 32-bit, 64-bit, Windows® 8.1 Pro 32-bit, 64-bit, Windows® 10 Pro 32-bit, 64-bit
CPU	Intel® Core i5 2.7GHz or higher (recommended)
Memory	At least 2 GB (4 GB or more recommended)
Hard disk	20 GB of available hard disk space At least 10 GB of available disk space is required on the system drive (drive where the OS is installed) for database.
Display	Display hardware capable of displaying 1,280 x 768 pixels/16-bit color or better
Other	Two USB ports required for protection key if used. Not necessary for electronic license. USB or serial port required for connection to instrument.
Compatible Instruments	
Models	CM-25cG, CM-2500c, CM-M6
Features	
Color space	L*a*b*, L*C*h, Lab99, LCh99, XYZ, Hunter Lab, Yxy, L*u*v', L*u*v*, and their color differences. Munsell C, Munsell D65
Index	MI, Color assessment, Gloss (CM-25cG), FF (CM-M6), WI (CIE 1982), Tint (CIE 1982), WI (ASTM E313-73), WI (Hunter), YI (ASTM E313-73), YI (ASTM D1925), WI (ASTM E313-98, Berger, Taube, Stensby, Ganz), YI (ASTM E313-98, DIN 6167), WB (ASTM E313-73), Tint (ASTM E313-98, Ganz), Opacity (ISO 2471, TAPPI T425 89% White Plate), Haze (ASTM D1003-97), and their differences, user equation, Standard Depth (ISO 105.A06), Brightness (TAPPI T452, ISO 2470), Density (Status A, Status T), Dominant Wavelength, Excitation Purity, RXRYRZ555, Strength (Tristimulus XYZ, Pseudo tristimulus XYZ), Staining degree (ISO 105.A04E), Staining degree rating (ISO 105.A04E), NC#, NC# Grade, Ns, Ns Grade, Grey Scale (ISO 105.A05), Grey Scale Rating (ISO 105.A05), K/S strength (Apparent (ΔE^*_{ab} , ΔL^* , ΔC^* , ΔH^* , Δa^* , Δb^*), Maximum absorption, total wavelength, user wavelength) Note on Haze (ASTM D 1003-97): With some instrument types, the illumination/observation system may not satisfy the definition of Haze (ASTM D 1003-97). However, this presents no problem as long as the value is used as a relative value.
Color difference formula	ΔE^*_{ab} (CIE 1976), ΔE^*_{94} (CIE 1994) and each component of lightness, saturation and hue, E_{00} (CIE DE2000) and each component of lightness, saturation and hue, ΔE_{99} (DIN 99), ΔE (Hunter), CMC (l:c) and each component of lightness, saturation and hue, FMC-2, NBS 100, NBS 200, ΔEc (degree) (DIN 6175-2), ΔEp (degree) (DIN 6175-2)
Observer	2° or 10° Standard Observer
Illuminants	A, C, D50, D55, D65, D75, F2, F6, F7, F8, F10, F11, F12, U50, ID50, ID65
Graph display	Spectral graph (reflectance, transmittance, K/S, Absorbance and its differences), L*a*b* absolute value, $\Delta L^*a^*b^*$ (color difference, MI), Hunter Lab absolute value, Hunter Δlab (color difference), Trend chart of each color space and color difference formula value, Pseudo color display
Instrument control	Measurement/calibration: Automatic averaging measurement: 2 to 30 measurements Manual averaging measurements: User-determined number of times (The standard deviation and average for the color space selected for measurement are displayed.) Remote measurement List display/reading of sample/target data stored in instrument memory Writing of target data to instrument memory
Instrument diagnosis	Applicable instruments: CM-25cG, CM-M6 Checked characteristics : Repeatability, reproducibility, lamp output (CM-25cG)
Target data	Target data can be registered. Main target and working targets under main targets can be used. Manual input of colorimetric or spectral target data possible.
Data list	Listing of target data and sample data Editing (delete, sort, average, copy & paste) Display of pass/fail ratio, Visual judgement result input function, Additional data information inputting/listing function
External I/O	Importing/exporting of data file (s) in original formats (Extension: mesx).
	Importing/exporting of template file (s) in original formats (Extension: mtpx).
	Importing of SpectraMagic NX data files (Extension: mes).
	Importing of SpectraMagic NX template files (Extension: mtp).
	Importing/exporting of data in text format. Saving of data in XML format. Exporting of data in Excel or PDF format. Copying of lists to clipboard.
Displayed Languages	(Selectable after installation) English, Japanese, German, French, Spanish, Italian, Portuguese, Turkish, Russian, Polish, Simplified Chinese, and Traditional Chinese
Help	Manual, "Precise Color Communication" Tutorial
Other	
Screen display	Number of files that can be opened simultaneously: 10 Number of data that can be stored in a file: 10,000 Instrument detailed status window.

: Available on Professional Edition only

- Windows® is a trademark or registered trademark of Microsoft Corporation in the USA and other countries.
- Intel® Core is a trademark or registered trademark of Intel Corporation in the USA and other countries.
- Displays shown are for illustration purpose only.

- The specifications and appearance shown herein are subject to change without notice.
- KONICA MINOLTA, the Konica Minolta logo and symbol mark, "Giving Shape to Ideas" and SpectraMagic are registered trademarks or trademarks of Konica Minolta, Inc.



SAFETY PRECAUTIONS

For correct use and for your safety, be sure to read the instruction manual before using the product.

KONICA MINOLTA, INC.
Konica Minolta Sensing Americas, Inc.
Konica Minolta Sensing Europe B.V.

Osaka, Japan
New Jersey, U.S.A.
European Headquarter / BENELUX
German Office
French Office
UK Office
Italian Office
Swiss Office
Nordic Office
Polish Office
SE Sales Division
Beijing Office
Guangzhou Office
Chongqing Office
Qingdao Office
Wuhan Office

Konica Minolta (CHINA) Investment Ltd.

Konica Minolta Sensing Singapore Pte Ltd.
Konica Minolta Sensing Korea Co., Ltd.

Addresses and telephone/fax numbers are subject to change without notice. For the latest contact information, please refer to the KONICA MINOLTA Worldwide Offices web page :

Phone : 888-473-2656 (in USA), 201-236-4300 (outside USA)
Nieuwegein, Netherlands
München, Germany
Roissy CDG, France
Warrington, United Kingdom
Cinisello Balsamo, Italy
Dietikon, Switzerland
Västra Frölunda, Sweden
Wrocław, Poland
Shanghai, China
Beijing, China
Guangdong, China
Chongqing, China
Shandong, China
Hubei, China
Singapore
Goyang-si, Korea

Phone : +31 (0) 30 248-1193
Phone : +49 (0) 89 4357 156 0
Phone : +33 (0) 1 80 11 10 70
Phone : +44 (0) 1925 467300
Phone : +39 02849488.00
Phone : +41 (0) 43 322-9800
Phone : +46 (0) 31 7099464
Phone : +48 (0) 71 73452-11
Phone : +86- (0) 21-5489 0202
Phone : +86- (0) 10-8522 1551
Phone : +86- (0) 20-3826 4220
Phone : +86- (0) 23-6773 4988
Phone : +86- (0) 532-8079 1871
Phone : +86- (0) 27-8544 9942
Phone : +65 6563-5533
Phone : +82 (0) 2-523-9726

Fax : 201-785-2482
Fax : +31 (0) 30 248-1280
Fax : +49 (0) 89 4357 156 99
Fax : +33 (0) 1 80 11 10 82
Fax : +44 (0) 1925 711143
Fax : +39 02849488.30
Fax : +41 (0) 43 322-9809
Fax : +48 (0) 71 734 52 10
Fax : +86- (0) 21-5489 0005
Fax : +86- (0) 10-8522 1241
Fax : +86- (0) 20-3826 4223
Fax : +86- (0) 23-6773 4799
Fax : +86- (0) 532-8079 1873
Fax : +86- (0) 27-8544 9991
Fax : +65 6560-9721
Fax : +82 (0) 31-995-6511



Certificate No : LRO 0960094/A
Registration Date : March 3, 1995



Certificate No : JOA-E-80027
Registration Date : March 12, 1997

<http://konicaminolta.com/instruments/network>